



INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(51) International Patent Classification⁶ :

A61B 5/08

A1

(11) International Publication Number:

WO 97/35518

(43) International Publication Date:

2 October 1997 (02.10.97)

(21) International Application Number: PCT/US97/04825

(22) International Filing Date: 24 March 1997 (24.03.97)

(30) Priority Data:

08/623,562

28 March 1996 (28.03.96)

US

(71) Applicant: INDIANAPOLIS CENTER FOR ADVANCED RESEARCH, INC. [US/US]; 635 Barnhill Drive, MS 313, Indianapolis, IN 46202 (US).

(72) Inventors: SANGHVI, Narendra T.; 818 Culpeper Court, Indianapolis, IN 46227 (US). BIHRLE, Richard; 8570 Twin Pointe Circle, Indianapolis, IN 46236 (US). FRY, Francis, J.; 414 West Spring Lake Boulevard, Port Charlotte, FL 33952 (US).

(74) Agents: CONARD, Richard, D. et al.; Barnes & Thornburg, 1313 Merchants Bank Building, 11 South Meridian Street, Indianapolis, IN 46204 (US).


(81) Designated States: AU, CA, JP, KR, MX, NZ, European patent (AT, BE, CH, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE).

Published*With international search report.**Before the expiration of the time limit for amending the claims and to be republished in the event of the receipt of amendments.*

(54) Title: FOCUSSED ULTRASOUND TISSUE TREATMENT METHOD

(57) Abstract

A method of treatment of tissue (136) with focussed ultrasound comprises placing adjacent the tissue (136) to be treated a reflector of ultrasound or an ultrasound energy conversion device (128) which converts received ultrasound energy to heat, stores the heat and then releases the heat over time into the tissue (136) to be treated. An ultrasound transducer (120) is then oriented with its focal point (142) adjacent the reflector or ultrasound energy conversion device (128). The tissue (136) is then irradiated with high intensity focussed ultrasound while the reflector or ultrasound energy conversion device (128) is in place.

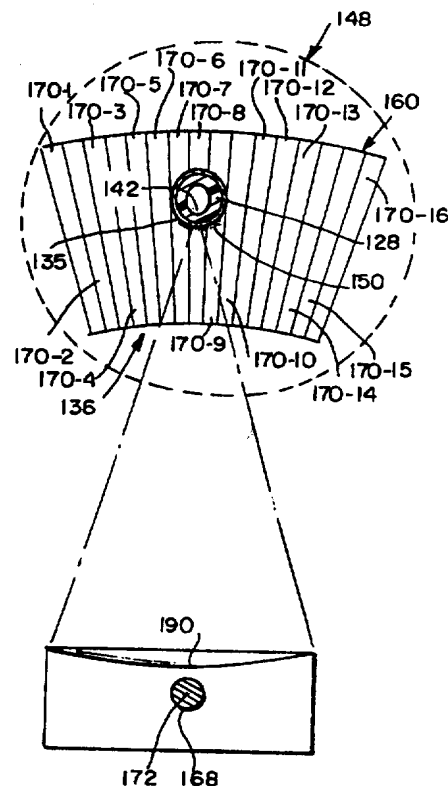

FOR THE PURPOSES OF INFORMATION ONLY

Codes used to identify States party to the PCT on the front pages of pamphlets publishing international applications under the PCT.

AL	Albania	ES	Spain	LS	Lesotho	SI	Slovenia
AM	Armenia	FI	Finland	LT	Lithuania	SK	Slovakia
AT	Austria	FR	France	LU	Luxembourg	SN	Senegal
AU	Australia	GA	Gabon	LV	Latvia	SZ	Swaziland
AZ	Azerbaijan	GB	United Kingdom	MC	Monaco	TD	Chad
BA	Bosnia and Herzegovina	GE	Georgia	MD	Republic of Moldova	TG	Togo
BB	Barbados	GH	Ghana	MG	Madagascar	TJ	Tajikistan
BE	Belgium	GN	Guinea	MK	The former Yugoslav Republic of Macedonia	TM	Turkmenistan
BF	Burkina Faso	GR	Greece			TR	Turkey
BG	Bulgaria	HU	Hungary	ML	Mali	TT	Trinidad and Tobago
BJ	Benin	IE	Ireland	MN	Mongolia	UA	Ukraine
BR	Brazil	IL	Israel	MR	Mauritania	UG	Uganda
BY	Belarus	IS	Iceland	MW	Malawi	US	United States of America
CA	Canada	IT	Italy	MX	Mexico	UZ	Uzbekistan
CF	Central African Republic	JP	Japan	NE	Niger	VN	Viet Nam
CG	Congo	KE	Kenya	NL	Netherlands	YU	Yugoslavia
CH	Switzerland	KG	Kyrgyzstan	NO	Norway	ZW	Zimbabwe
CI	Côte d'Ivoire	KP	Democratic People's Republic of Korea	NZ	New Zealand		
CM	Cameroon	KR	Republic of Korea	PL	Poland		
CN	China	KZ	Kazakhstan	PT	Portugal		
CU	Cuba	LC	Saint Lucia	RO	Romania		
CZ	Czech Republic	LI	Liechtenstein	RU	Russian Federation		
DE	Germany	LK	Sri Lanka	SD	Sudan		
DK	Denmark	LR	Liberia	SE	Sweden		
EE	Estonia			SG	Singapore		

FOCUSSED ULTRASOUND TISSUE TREATMENT METHODTechnical Field

5 This invention relates to ultrasound tissue ablation. It is disclosed in the context of prostate ablation, but it is believed to be useful in other applications as well.

Background Art

10 The efficacy of ultrasound as a medium for non-invasive or minimally invasive tissue removal has been established. There are, for example the disclosures of U.S. Patents: 4,586,512; 4,620,546; 4,658,828; 4,858,613; 4,951,653; 4,955,365; 5,036,855; 5,054,470; 5,149,319; 15 5,215,680; and, 5,219,401. No representation is intended hereby that a thorough search of all material prior art has been conducted or that no more material prior art exists. Nor should any such representation be inferred.

In some applications, however, some portion of 20 the transmitted ultrasound energy is not applied to optimal effect. For example, it is known that in the transrectal ultrasound ablation of prostate tissue, such as in the treatment of benign prostatic hyperplasia (BPH), the posterior lesion (that is, the lesion that forms between 25 the depth at which the urethra passes through the prostate and the posterior surface of the prostate) is much more effective in relieving the symptoms of BPH than the anterior lesion (the lesion that forms between the depth at which the urethra passes through the prostate and the 30 anterior surface of the prostate). In this sense, the ultrasound energy that results in the anterior lesion is "wasted," although the anterior lesion is formed. If this energy could be reflected back posteriorly for integration with the energy that is absorbed by the posterior prostate, 35 the effectiveness of the ultrasound ablation treatment at relieving BPH symptoms would be enhanced.

Disclosure of Invention

Accordingly it is an object of this invention to provide methods and apparatus by which the effectiveness of ultrasound as a medium for tissue ablation is enhanced.

5 According to an aspect of the invention, a method of treatment of tissue with focussed ultrasound comprises placing adjacent the tissue to be treated a reflector of ultrasound, orienting an ultrasound transducer with its focal point adjacent the reflector and then irradiating the
10 tissue with focussed ultrasound while the reflector is in place.

 According to another aspect of the invention, a method of treatment of tissue with focussed ultrasound comprises placing adjacent the tissue to be treated an
15 ultrasound energy conversion device which converts received ultrasound energy to heat, stores the heat and then releases the heat over time into the tissue to be treated. An ultrasound transducer is oriented with its focal point adjacent the ultrasound energy conversion device. The
20 tissue is then irradiated with focussed ultrasound while the ultrasound energy conversion device is in place.

 Illustratively, the step of placing adjacent the tissue to be treated a reflector of ultrasound or an ultrasound energy conversion device comprises the step of
25 inserting a catheter comprising an ultrasound reflective material or ultrasound energy converting and heat storage material into a body lumen or orifice which lies adjacent the tissue to be treated.

 Additionally illustratively, the step of
30 inserting a catheter comprising an ultrasound reflective material or an ultrasound energy converting and heat storage material into a body lumen or orifice comprises the step of inserting a catheter containing red rubber into the body lumen or orifice.

35 Further illustratively, the step of inserting a catheter comprising an ultrasound reflective material or

-3-

ultrasound energy converting and heat storage material into a body lumen or orifice which lies adjacent the tissue to be treated comprises the steps of inserting a balloon catheter into the urethra to the depth of the bladder and
5 inflating the balloon in the bladder.

Additionally illustratively, the step of irradiating the tissue with ultrasound comprises irradiating the prostate with the high intensity focussed ultrasound.

10 Further illustratively, the step of orienting the ultrasound transducer with its focal point adjacent the reflector comprises the step of coupling the transducer through the rectal wall.

15 Brief Description of the Drawings

The invention may best be understood by referring to the following description and accompanying drawings which illustrate the invention. In the drawings:

20 Fig. 1 illustrates a step in the prior art transrectal high intensity focussed ultrasound (HIFU) ablation of a diseased prostate;

Fig. 2 illustrates a corresponding step to the one illustrated in Fig. 1, but performed according to the present invention;

25 Fig. 3 illustrates a much enlarged view of a detail of the step illustrated in Fig. 2;

Fig. 4 illustrates a view of the detailed illustration in Fig. 3 taken generally along section lines 4-4 of Fig. 3; and

30 Fig. 5 illustrates temperature profiles obtained with a system constructed and operated in accordance with the teachings of Figs. 2-4.

Modes of Practicing the Invention

35 A limitation on the effectiveness of HIFU as a treatment for BPH can best be appreciated by referring to

Fig. 1. An ultrasound transducer 20 in a coupling fluid 22 is inserted into the colon 24 of a sufferer of BPH directly behind the affected prostate 26. Numerous techniques for visualization of this region are known. Many systems for visualization employ the same transducer 20 in a low power, visualization mode for visualization of the prostate 26, and in a HIFU mode for subsequent ablation therapy. The visualization is usually accomplished with the aid of a urethral catheter (not shown) having a balloon end and an inflating lumen for inflating the balloon in the neck 32 of the bladder 34 to anchor the catheter. The catheter is visible in the visualizing intensity ultrasound generated by transducer 20.

After the visualization of the neck 32 of the bladder 34, the urethra 35 and surrounding diseased prostate 26 has been completed and the transducer 20 is oriented for treatment of the prostate 26, the balloon is deflated, the catheter is removed and the HIFU treatment of the prostate 26 for BPH commences according to a treatment format established by the treating physician. The lesion 36 which results from the application of the HIFU is somewhat elongated, with a somewhat larger posterior portion 38 of the lesion 36 lying between the rectal wall 40 and the focal zone 42 of the ultrasound beam 44 in the vicinity of (indeed here at) the urethra 35. A somewhat smaller portion 48 of the lesion 36 lies anterior to the urethra 35 toward the lower front of the abdomen. Although the HIFU energy which is absorbed by the prostate 26 anterior to the urethra 35 does result in an anterior lesion 48, the relief of BPH symptoms afforded by the anterior lesion 48 is not as great as the relief afforded by the posterior lesion 38.

Referring now to Figs. 2, 3 and 4, according to the invention, an ultrasound transducer 120 in a coupling fluid 122 is inserted into the colon 124 of a sufferer of BPH directly behind the affected prostate 126.

-5-

Visualization of the treatment field is accomplished with the aid of a urethral catheter 128 having a balloon end 130 and an inflating lumen for inflating the balloon 130 in the neck 132 of the bladder 134 and to anchor the catheter 128.

5 The catheter 128 is visible in the visualizing intensity ultrasound for transducer 120. After the visualization of the urethra 135 and surrounding diseased prostate 126 has been completed and the transducer 120 is oriented for treatment of the prostate 126, the catheter 128 is not

10 removed. Rather the HIFU treatment of the prostate 126 for BPH commences with the catheter 128 in place in the urethra 135 according to a treatment format established by the treating physician.

The lesion 136 which results from the application

15 of the HIFU is limited almost exclusively by the presence of catheter 128 to between the rectal wall 140 and the focal zone 142 of the ultrasound beam 144 in the vicinity of the surface of catheter 128. In this way, the HIFU incident on the catheter 128 is reflected posteriorly and

20 combines with the direct HIFU to achieve an effective lesion 136, generally with lower input power to transducer 120. Almost no HIFU energy is transmitted to, or absorbed by, the prostate 126 anterior to the urethra 135. Therefore, there is no "wasted" lesion in region 148. The

25 relief of BPH symptoms is delivered more effectively and with lower input power by limiting the lesion to region 136. This effect is further enhanced by what appears to be cavitation bubble "seeding" of region 136 adjacent catheter 128 and urethra 135. As the HIFU is applied, cavitation

30 bubbles 150 appear readily in this area. The cavitation bubbles trap both some HIFU energy incident on catheter 128 and some HIFU energy reflected from catheter 128, and release this trapped energy back into the posterior lesion prostate tissue as they rupture, enhancing the efficiency

35 of the HIFU at producing the posterior lesion 136. Microscopic imperfections in the outer wall of catheter 128

-6-

are believed to contribute to this cavitation bubble enhancement phenomenon.

Various kinds of catheters 128 have been employed. Suitable catheters include Surgicot™ red rubber catheters, Dow Corning Silastic® Foley catheters, Olbert urological catheters, Bardex Foley catheters and Baxter urological catheters.

A suitable treatment format can best be appreciated by referring to Figs. 2-5. A region of the prostate 126 to be treated is divided into a grid 160, with sections 162-1, 162-2 . . . 162-12 spaced uniformly along the adjacent rectal wall 140 capable of being individually addressed for HIFU treatment by moving the transducer 120 in the directions indicated by double ended arrow 166 into and out of the colon 124. Uniformly angularly spaced sectors 170-1, 170-2 . . . 170-16 are capable of being individually addressed by rotation of the treatment transducer 120 about its axis 172 on drive shaft 168, as indicated by double ended arrow 174. A code wheel (not shown) can be fixed on the shaft 168 for reading the angular orientation of the transducer 120 in accordance with known principles. See, for example, U.S. Patent 4,664,121. In this manner, the tissue of the prostate 126 in the treatment region 160 can be treated, one longitudinal 162-1, . . . 162-12 and angular 170-1, . . . 170-16 sector at a time. Such a treatment format will result in temperature profiles illustrated in Fig. 5. Body temperature is illustrated by curve 180. As will be appreciated body temperature remote from the treatment site 160 is unaffected by the treatment. The temperature of the coupling liquid, in this case, deionized, degassed water in the transducer probe 182 is illustrated by curve 184. The reason for the discontinuity at about 39 minutes of the treatment regimen is that an external coupling liquid circulation circuit (not shown) was activated at that time, resulting in circulation of the coupling liquid through the

external circuit and the resultant cooling of the coupling liquid. Curve 188 is a temperature profile of the rectal wall 140. The rectal wall 140 lies in the near field of the treatment transducer 120, that is, between the emitting surface 190 of the treatment transducer 120 and the focal zone 142 of the treatment transducer 120. Curve 196 is a temperature profile of the surface of the catheter 128. The spikes in the various temperature profiles occur when the focal zone 142 is very close to the various thermocouples used to generate the temperature profiles. Curve 196 clearly establishes the efficacy of the treatment method of the present invention employing the HIFU energy conversion, heat retention and heat radiation capability of catheter 128 when catheter 128 is left in place during the HIFU treatment.

Because the treatment thermal dosage is proportional to $\Sigma T\Delta t$ where T is any elevated temperature at which tissue is maintained and Δt is the time during which the tissue is maintained at that temperature, raising the temperature of the tissue-catheter 128 surface interface, both by ultrasound absorption and reradiation, and by reflection of ultrasound, will assure more complete tissue destruction.

The above-noted materials are illustrative of materials that absorb ultrasound, convert it into heat and store and radiate the heat into the surrounding tissue. Polymers generally are noted for exhibiting these same characteristics, that is, enhanced effects of HIFU exposure of tissue. These effects can be further augmented by the use of Albunex or other microbubble or microbubble production-enhancing materials. These materials can be used to enhance cavitation of liquids in the tissue, making the benefits of cavitation as a tissue ablation mechanism more accessible at lower applied HIFU power densities. Additionally, the presence of the red rubber, Silastic®, and other polymer material catheters 128 promotes

cavitation even without the presence of other cavitation-inducing agents at much lower applied HIFU powers (sometimes reduced by half or more). The mismatched foreign material and tissue acoustic impedances produce larger reflected energy as well, accounting for some of the enhanced tissue ablation demonstrated by the presence of these foreign material catheters 128 in the urethra 135. The foreign material provides an enhanced environment for cavitation at the foreign material-tissue interface. The increased energy released at this interface gives rise to higher pressure and shock waves, disintegrating the tissue and mechanically destroying the tissue in a predictable manner. This promotes sloughing off of the tissue in the treatment zone 136, providing more immediate and lasting relief of BPH symptoms.

Also, when the transducer 120 is being used in the visualization mode, because lower applied power can induce cavitation and because cavitation bubbles are extremely echogenic, the treatment site 136 is much more readily visualized with the foreign object 128 in place. With the foreign object 128 in place in the body, differences in ultrasound tissue absorption coefficients become much less critical in the application of sufficient HIFU to achieve ablation. Thus, the effects of variations in the tissues encountered in the near field between the transducer 120 and the focal zone 142 in a patient, or from patient to patient, on patient treatment regimens and formats are reduced.

CLAIMS:

1. A method of treatment of tissue with focussed ultrasound comprising placing adjacent the tissue to be treated a reflector of ultrasound, orienting an ultrasound transducer with its focal point adjacent the reflector and then irradiating the tissue with focussed ultrasound while the reflector is in place, the reflector reflecting energy into the tissue to aid the focussed ultrasound in treating the tissue.
2. The method of claim 1 wherein the step of placing adjacent the tissue to be treated a reflector of ultrasound comprises the step of inserting a catheter comprising an ultrasound reflective material into a body lumen or orifice which lies adjacent the tissue to be treated.
3. The method of claim 2 wherein the step of inserting a catheter comprising an ultrasound reflective material into a body lumen or orifice comprises the step of inserting a catheter containing red rubber into the body lumen or orifice.
4. The method of claim 2 wherein the step of inserting a catheter comprising an ultrasound reflective material into a body lumen or orifice which lies adjacent the tissue to be treated comprises the steps of inserting a balloon catheter into a urethra to the depth of a bladder and inflating the balloon in the bladder.
5. The method of claim 4 wherein the step of irradiating the tissue with ultrasound comprises irradiating a prostate with the high intensity focussed ultrasound.
6. The method of claim 5 wherein the step of orienting the ultrasound transducer with its focal point adjacent the reflector comprises the step of coupling the transducer through a rectal wall.
7. A method of treatment of tissue with

-10-

focussed ultrasound comprising placing adjacent the tissue to be treated an ultrasound energy conversion device which converts received ultrasound energy to heat, stores the heat and then releases the heat over time into the tissue to be treated, orienting an ultrasound transducer with its focal point adjacent the ultrasound energy conversion device and then irradiating the tissue with focussed ultrasound while the ultrasound energy conversion device is in place, the energy conversion device releasing the heat over time into the tissue to be treated, aiding the focussed ultrasound in treating the tissue.

8. The method of claim 7 wherein the step of placing adjacent the tissue to be treated an ultrasound energy conversion device comprises the step of inserting a catheter comprising an ultrasound energy converting material into a body lumen or orifice which lies adjacent the tissue to be treated.


9. The method of claim 8 wherein the step of inserting a catheter comprising an ultrasound energy converting material into a body lumen or orifice comprises the step of inserting a catheter containing red rubber into the body lumen or orifice.

10. The method of claim 8 wherein the step of inserting a catheter comprising an ultrasound energy converting material into a body lumen or orifice which lies adjacent the tissue to be treated comprises the steps of inserting a balloon catheter into a urethra to the depth of a bladder and inflating the balloon in the bladder.

11. The method of claim 10 wherein the step of irradiating the tissue with ultrasound comprises irradiating a prostate with the focussed ultrasound.

12. The method of claim 11 wherein the step of orienting the ultrasound transducer with its focal point adjacent the ultrasound energy conversion device comprises the step of coupling the transducer through a rectal wall.


1/4

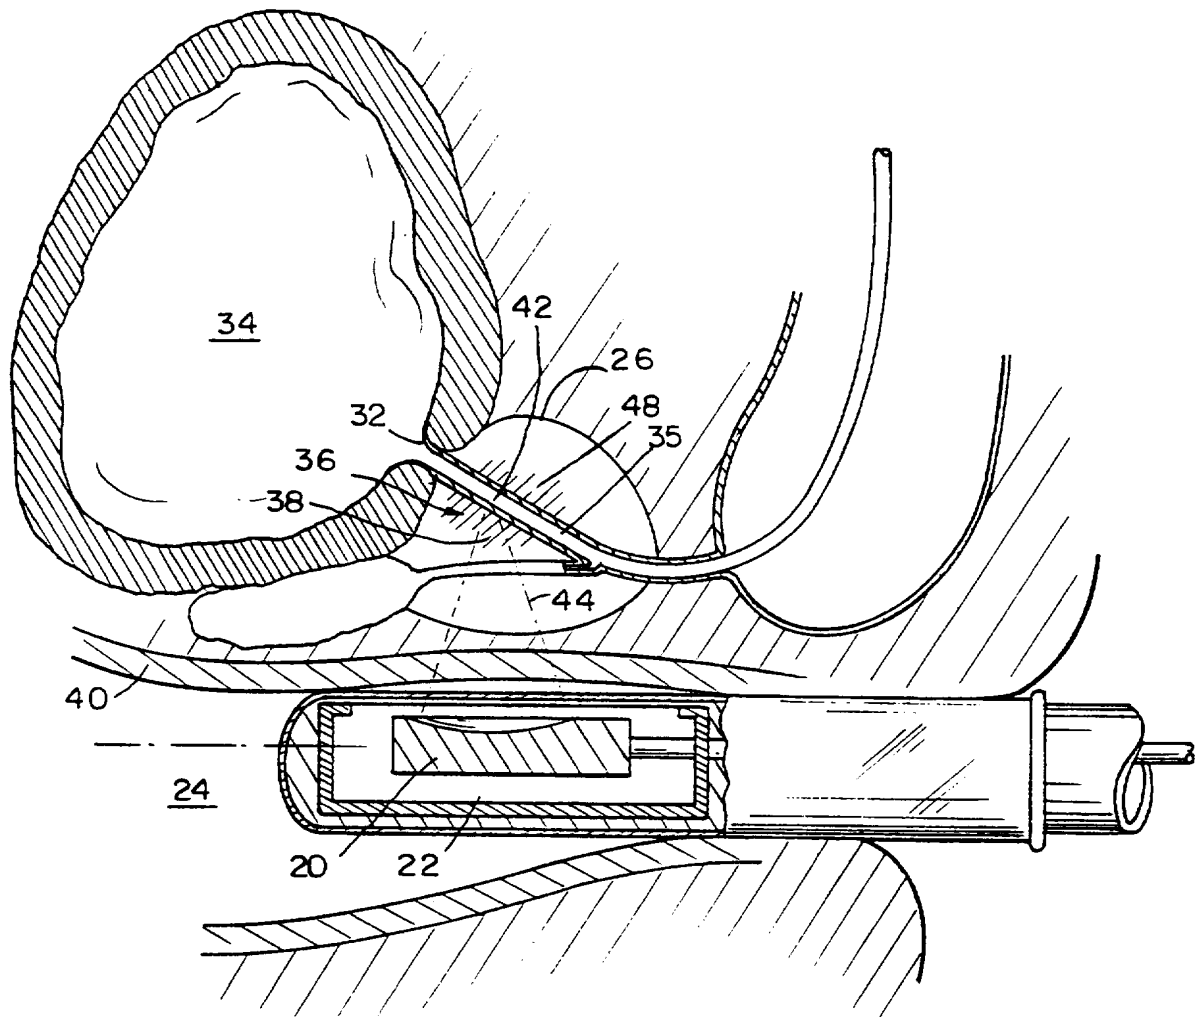

PRIOR ART

FIG. 1

2/4

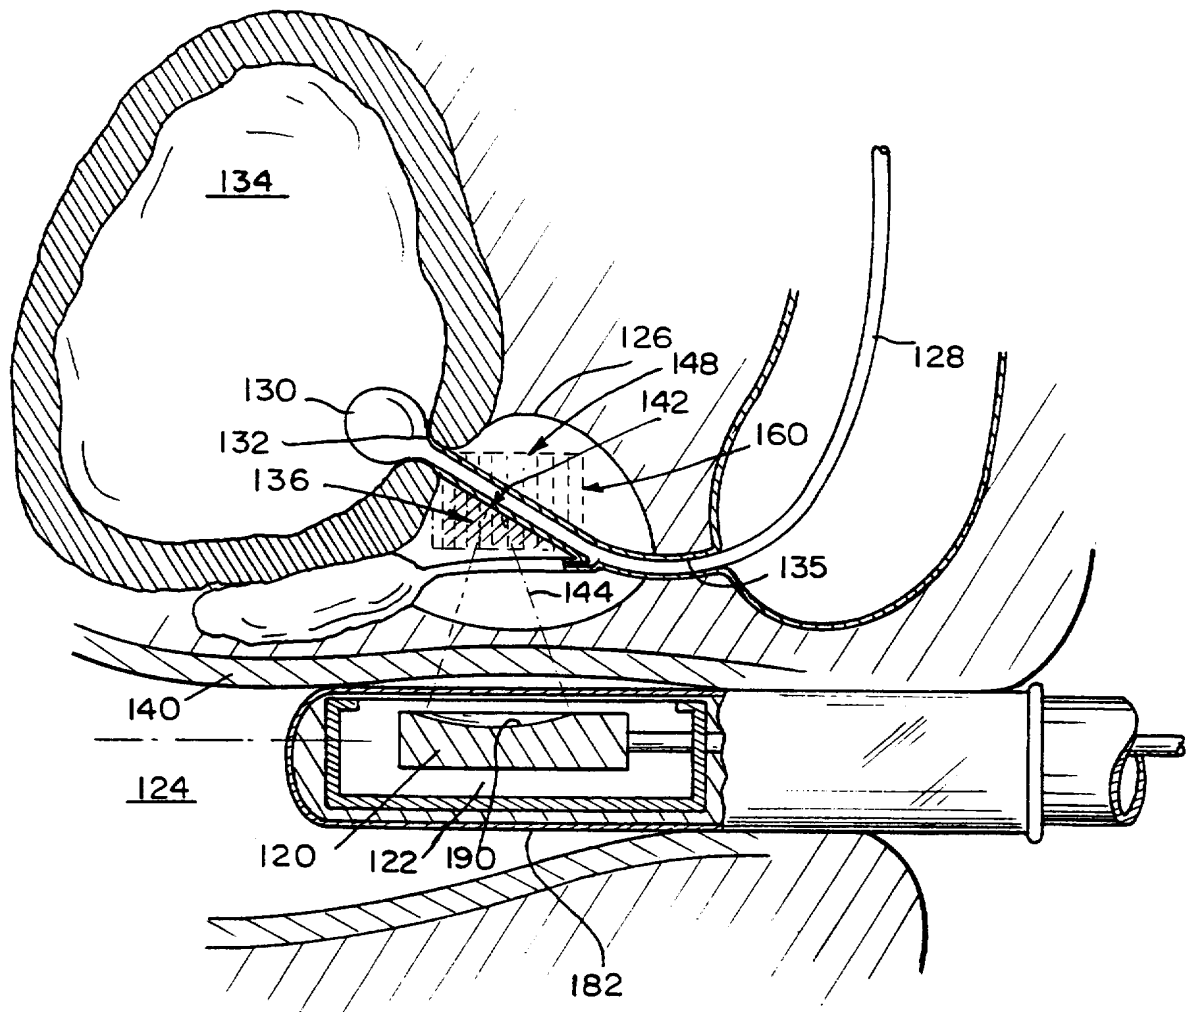*FIG 2*


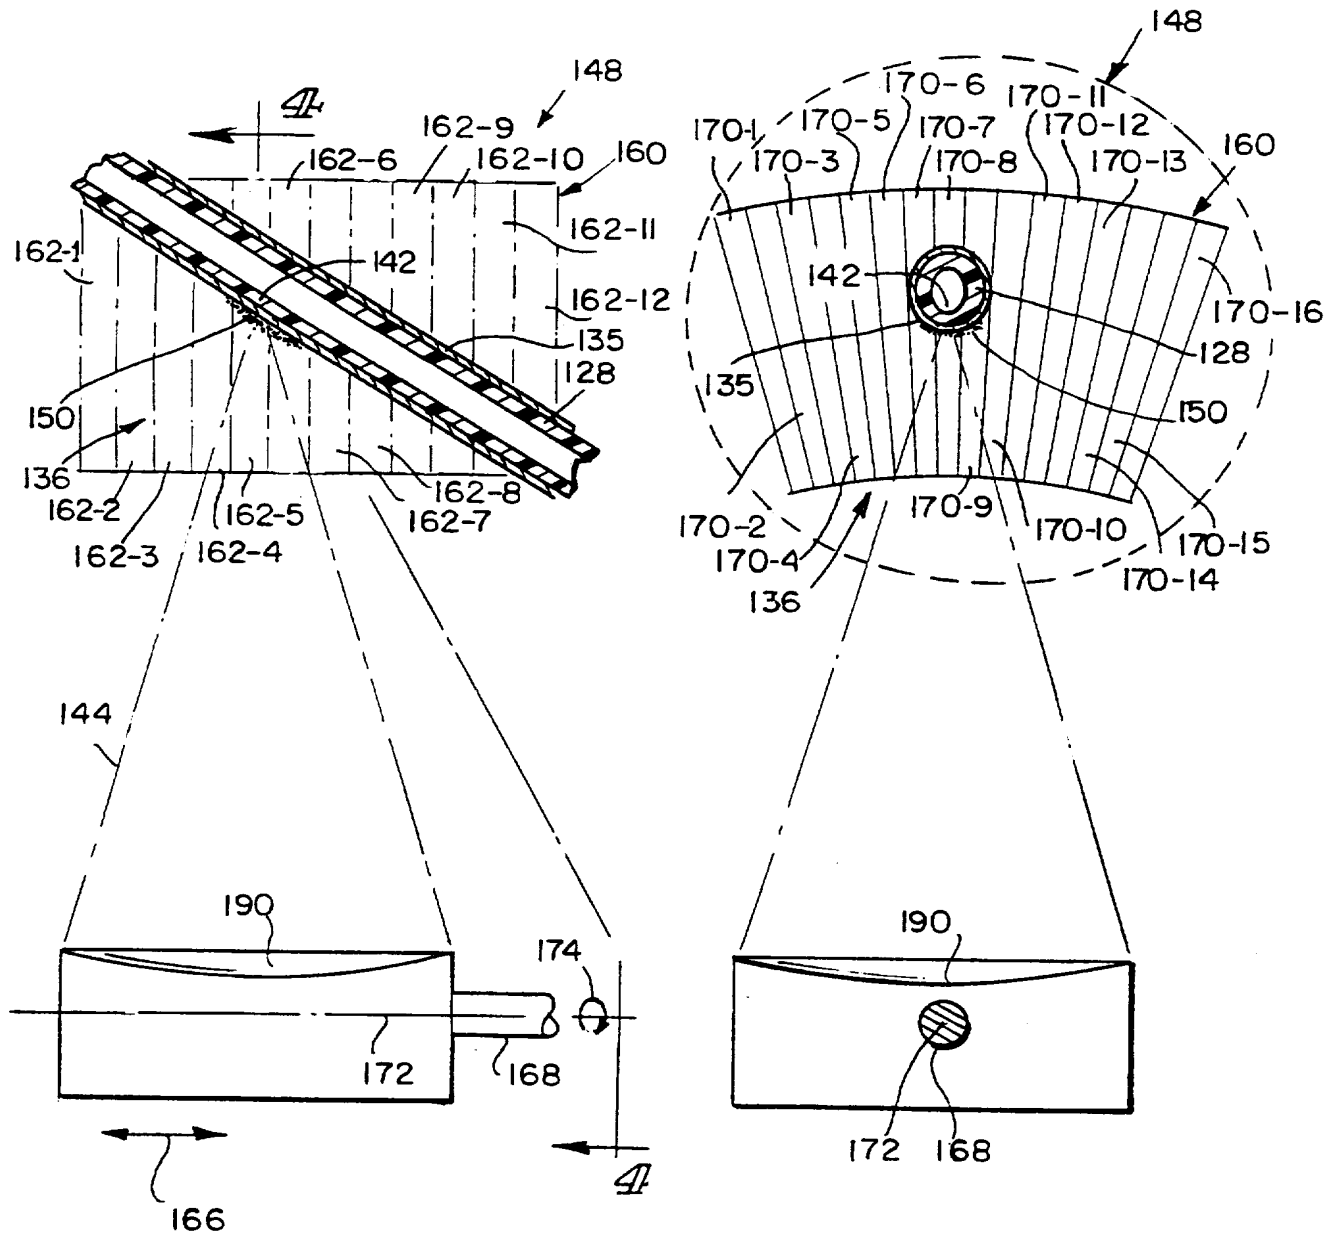


FIG. 3

FIG. 4

4 / 4

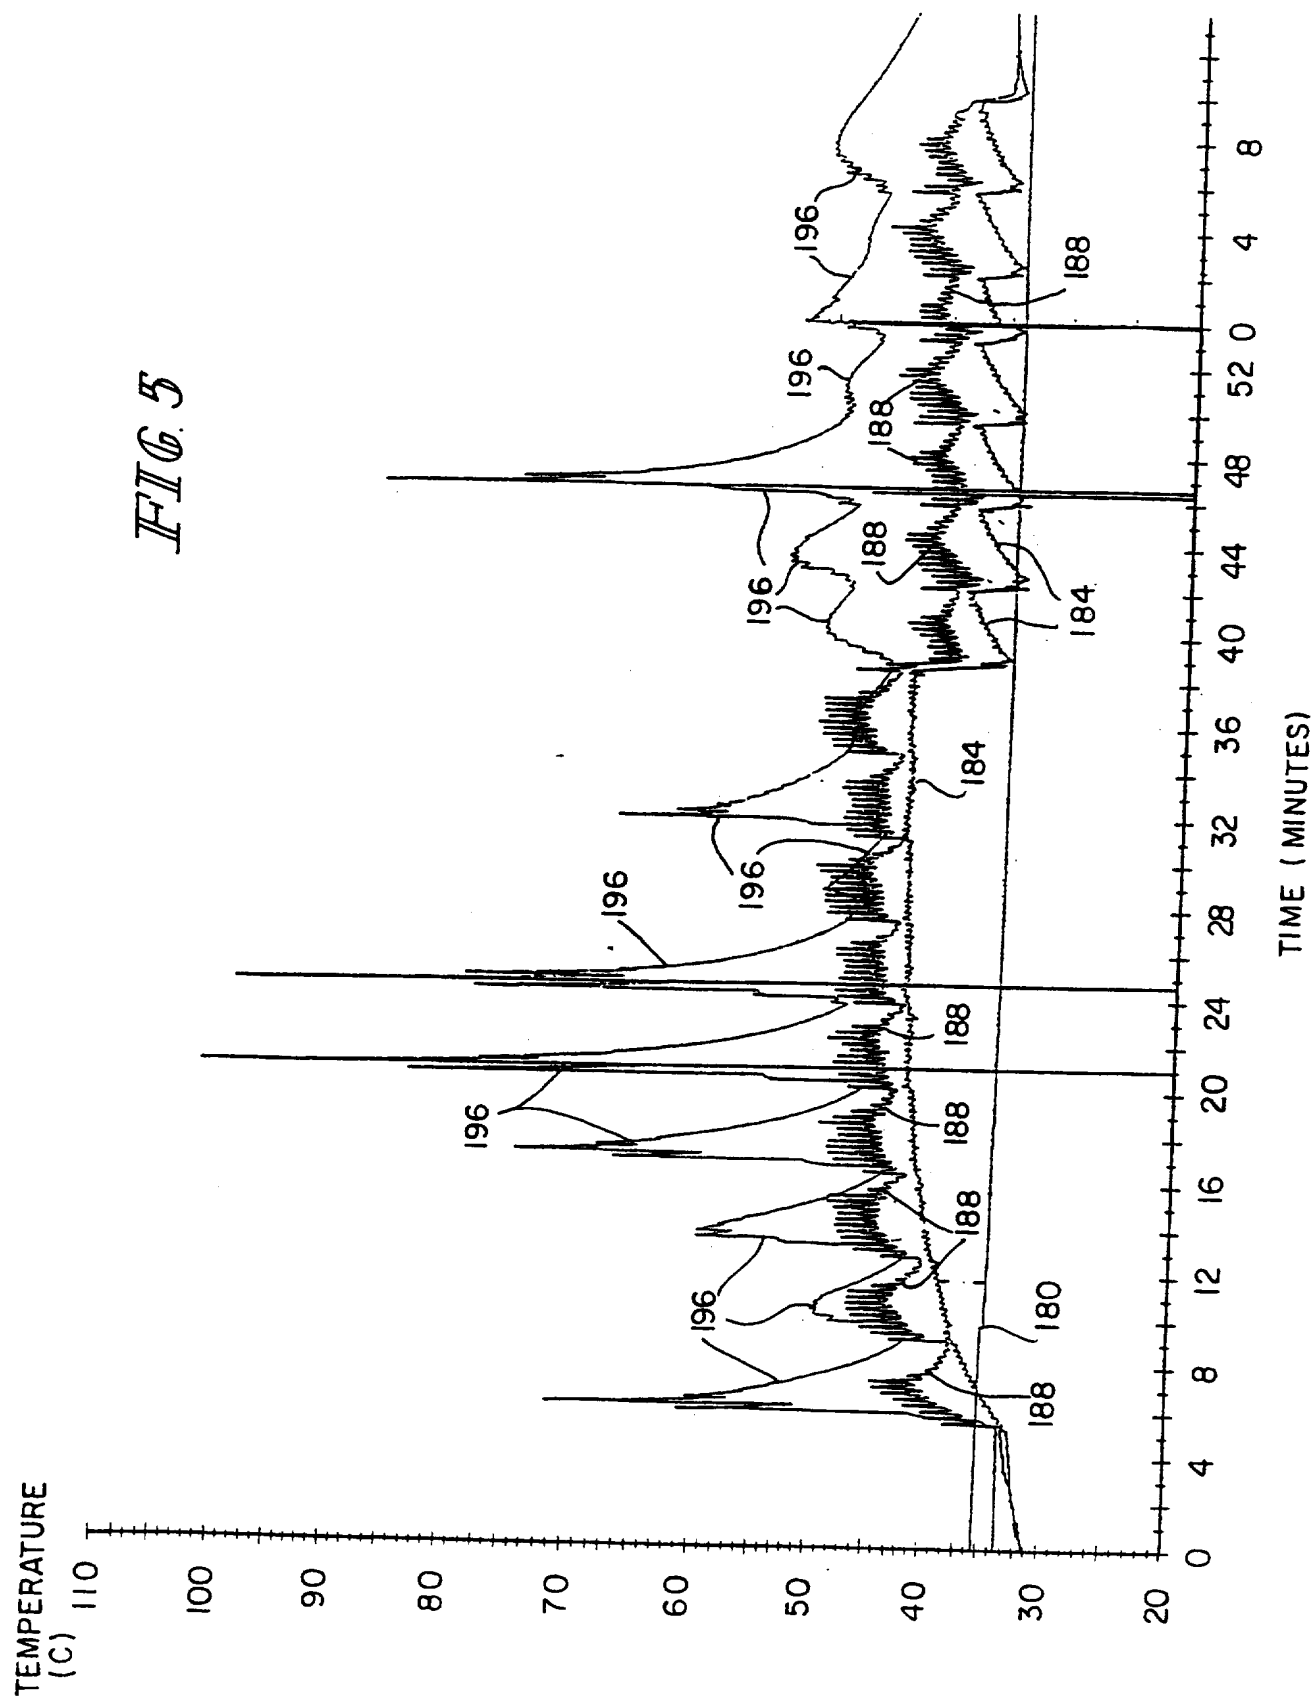

INTERNATIONAL SEARCH REPORT

International application No.

PCT/US97/04825

A. CLASSIFICATION OF SUBJECT MATTER

IPC(6) : A61B 5/08

US CL : 128/660.01, 660.03; 607/97

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

U.S. : 128/660.01, 660.03 ; 607/96, 97, 113, 114

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	US 5,470,350 A (BUCHHOLTZ et al) 28 November 1995, entire document.	1-12
A	US 5,474,071 A (CHAPELON et al) 12 December 1995, entire document.	1-12
A	US 5,234,004 A (HASCOET et al) 10 August 1993, entire document.	1-12

☐ Further documents are listed in the continuation of Box C.
 ☐ See patent family annex.

* Special categories of cited documents:	"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention
"A" document defining the general state of the art which is not considered to be of particular relevance	"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone
"E" earlier document published on or after the international filing date	"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art
"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)	"Z" document member of the same patent family
"O" document referring to an oral disclosure, use, exhibition or other means	
"P" document published prior to the international filing date but later than the priority date claimed	

Date of the actual completion of the international search

02 JULY 1997

Date of mailing of the international search report

23 JUL 1997

 Name and mailing address of the ISA/US
 Commissioner of Patents and Trademarks
 Box PCT
 Washington, D.C. 20231

Facsimile No. (703) 305-3230

Authorized officer

STEPHEN HUANG

Telephone No. (703) 308-3399